



Allow the kit and specimen to come to room temperature (65°F-86°F/18°C-30°C) prior to testing.  
**AVOID PLACING ANYTHING IN THE MOUTH 10 MINUTES PRIOR TO TESTING.**

- 1** Remove the test cube and the sponge collector from the foil pouch by tearing at the notch. Place the test cube upright on a level surface.

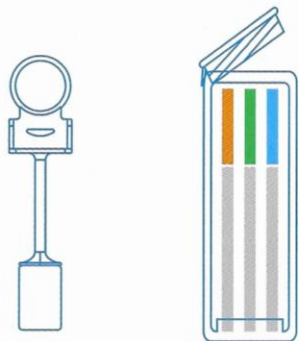


- 2** Put the sponge end of the collector in your mouth to collect oral fluid for about 7 minutes or until the sponge is fully saturated by oral fluid. Do not chew, bite or suck the sponge. If the amount of oral fluid does not make the sponge fully saturated within 7 minutes, repeat the collection using one additional sponge collector provided, beginning with Step 1.

**Note:** In case of the dry mouth, do not swallow oral fluid during collection.

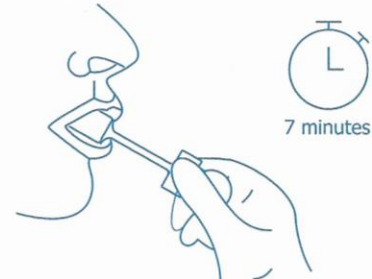

- 3** Open the test cube and place the fully saturated sponge collector inside the test cube. Press the sponge collector down firmly until it reaches the bottom of the test cube, then close the cube lid tightly while compressing the collector. Keep test cube upright on flat surface and follow Step 4.

**Note:** Make sure the sponge collector is inserted vertically and the handle of collector is put into the clamp.

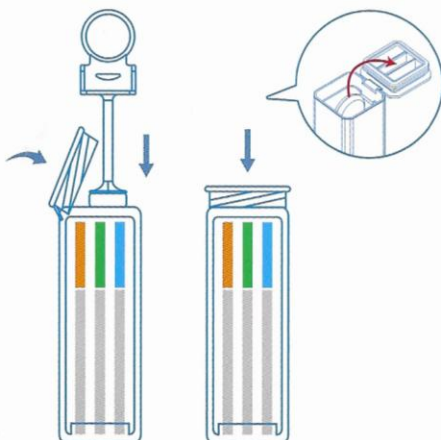

- 4** **1. Interpreting Alcohol Test Result:**

Read result at 2 minutes. Do not read after 2 minutes.


**NEGATIVE:** No color changes on reaction pad.

**POSITIVE:** Compare the color of reaction pad with provided color chart to estimate the approximate blood alcohol level.


- 2. Interpreting Drug Test Results:**

Read results at 5 minutes. Do not read after 5 minutes.

### Drug Test Results

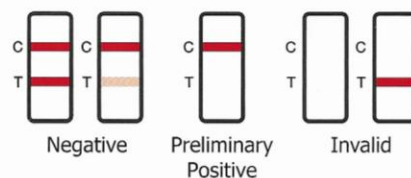

### Blood Alcohol Concentration



**NOTE:** Results after more than 2 minutes may be not accurate